



7863 La Mesa Blvd Suite 204 La
Mesa, CA 91942
619.724.6040
apexsleep.com

Dr. Name

Dr. Signature

Due Date

Patient name

Address

Phone

Device

Pro Avera

Hush Pro Auto

Patient measurements

Example

Maximum retrusion

-4 mm

mm

Dental midline deviation in occlusion

Maximum protrusion

6mm

mm

To the right


To the left

mm


None

Type of Bite Provided


The appliance will be set at $\pm 60\%$ of the maximum protrusion to allow increment protrusion up to the maximum protrusion

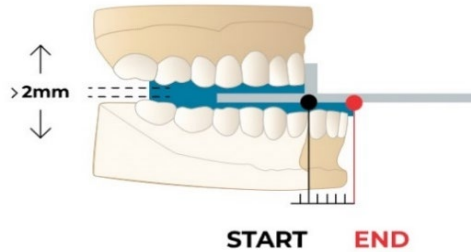

The appliance will be to start at the provided bite position, to allow incremental forward movement

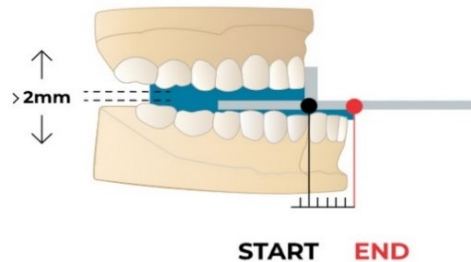

Select Fragile Teeth, Crown, Pontic & Implant Teeth

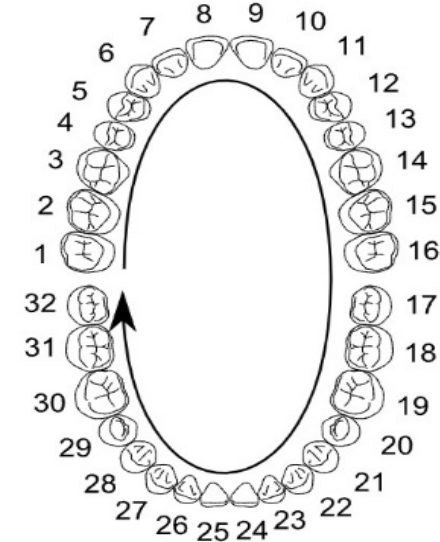

Vertical Spacing

Close or open to optimised the device

Keep it, call if major changes needed

Is Mandibular Protrusion Straight?

Yes

No

Observations